

2020

DATAMASTER

RECORD OF INSPECTION

MAINTENANCE

CALIBRATION



**Division of Criminal
Justice Services**

**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 138506, performed on November 04, 2020 by Office of Public Safety employee Joseph Iavarone, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance/calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Joshua Vinehout".

Digitally signed under ESRA
by Joshua Vinehout
on 11/12/2020 10:09 AM

**Joshua Vinehout
Supervisor of Public Safety Programs
Office of Public Safety**

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Solvay Village Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS Model: DATAMASTER DMT
Serial Number: 138506
Date: November 04, 2020

Reference Solution Lot Number: 20340
Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

| Test No | Test Result | Simulator Temperature |
|---------|-------------|--------------------------|
| 1 | 0.100 % | 33.99 degrees centigrade |
| 2 | 0.100 % | 33.99 degrees centigrade |
| 3 | 0.100 % | 33.99 degrees centigrade |
| 4 | 0.100 % | 33.99 degrees centigrade |

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 138506, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under
ESRA by Joseph Iavarone
on 11/4/2020 1:57 PM

Joseph Iavarone
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 44106

Reviewed by:



Digitally signed under
ESRA by Frank Sgarlata
on 11/5/2020 1:39 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Solvay Village Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS
Model: DATAMASTER DMT
Serial Number: 138506
Date: November 04, 2020

1. General Appearance and condition of this device -----: N/A
2. Check controls and indicators -----: OK
3. Check breath flow system -----: OK
4. Check printer operation -----: N/A
5. System cycles through all modes -----: OK
6. Record any repairs made to this instrument and list services provided: **CHECKED REMOTE OPERATION, RAN DIAGNOSTIC AND TECHNICIAN TESTS, VERIFIED CALIBRATION.**



Performed by:

Joseph Iavarone

Digitally signed under
ESRA by Joseph Iavarone
on 11/4/2020 1:57 PM

Joseph Iavarone
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 44106

Reviewed by:

Frank Sgarlata

Digitally signed under
ESRA by Frank Sgarlata
on 11/5/2020 1:39 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

SOLVAY VILLAGE
POLICE DEPT
DATAMASTER dmt: 138506

Date: 11/04/2020

Nominal = 0.100 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.000 | 13:06 |
| INTERNAL STANDARD | VERIFIED | 13:06 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.100 | 13:06 |
| BLANK TEST | 0.000 | 13:07 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.100 | 13:08 |
| BLANK TEST | 0.000 | 13:08 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.100 | 13:09 |
| BLANK TEST | 0.000 | 13:10 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.100 | 13:10 |
| BLANK TEST | 0.000 | 13:11 |

Average = 0.1000

Std Dev = 0.0000

Control Test Record

Serial Number: 138506

Test Date: 11/02/2020 17:22:14

Location: 190

SOLVAY VILLAGE POLICE DEPT.

Supervisor Information

First Name: Hunter

Last Name: Nerber

Permit: 48077

Agency: SOLVAY VILLAGE PD

Simulator Information

Lot: 20340

Nominal: 0.100

Test Results


Alcohol 1: 0.09 33.99

Alcohol 2: 0.09 33.99

Alcohol 3: 0.10 33.99

Solution Change:

Plot 1 of 3 < =>

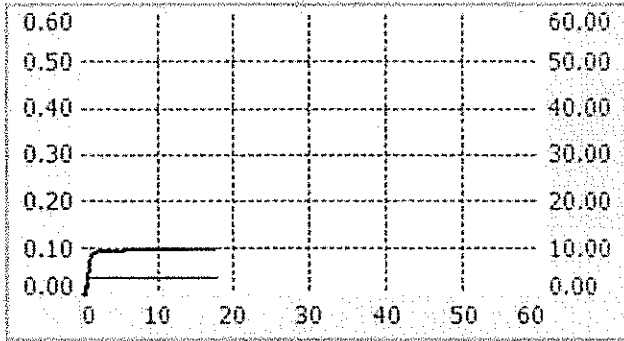

Status

Status Code:

Date Time:

Message:



Division of Criminal Justice Services

CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 138506, performed on May 29, 2020 by Office of Public Safety employee Joseph Iavarone, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Joshua Vinehout".

Digitally signed under
ESRA by Joshua Vinehout
on 6/5/2020 9:30 AM

Joshua Vinehout
Supervisor of Public Safety Programs
Office of Public Safety

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Solvay Village Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS Model: DATAMASTER DMT
Date: May 29, 2020 Serial Number: 138506

Reference Solution Lot Number: 19281
Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

| Test No | Test Result | Simulator Temperature |
|---------|-------------|--------------------------|
| 1 | 0.101 % | 34.00 degrees centigrade |
| 2 | 0.102 % | 34.00 degrees centigrade |
| 3 | 0.102 % | 34.00 degrees centigrade |
| 4 | 0.100 % | 34.00 degrees centigrade |

Reference Solution Lot Number: 20020
Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

| Test No | Test Result | Simulator Temperature |
|---------|-------------|--------------------------|
| 1 | 0.082 % | 33.99 degrees centigrade |
| 2 | 0.082 % | 34.00 degrees centigrade |
| 3 | 0.082 % | 34.00 degrees centigrade |
| 4 | 0.082 % | 34.00 degrees centigrade |

Reference Solution Lot Number: 19210
Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

| Test No | Test Result | Simulator Temperature |
|---------|-------------|--------------------------|
| 1 | 0.185 % | 34.00 degrees centigrade |
| 2 | 0.185 % | 34.00 degrees centigrade |
| 3 | 0.186 % | 34.00 degrees centigrade |
| 4 | 0.186 % | 34.00 degrees centigrade |

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 138506, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under
ESRA by Joseph Iavarone
on 5/29/2020 1:12 PM

Joseph Iavarone
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 44106

Reviewed by:



Digitally signed under
ESRA by Frank Sgarlata
on 6/1/2020 1:46 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Solvay Village Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS
Model: DATAMASTER DMT
Serial Number: 138506
Date: May 29, 2020


- 1. General Appearance and condition of this device -----: OK

- 2. Check controls and indicators -----: OK

- 3. Check breath flow system -----: OK

- 4. Check printer operation -----: OK

- 5. System cycles through all modes -----: OK

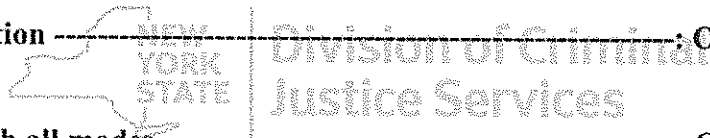

6. Record any repairs made to this instrument and list services provided: **INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES, PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**

Performed by:

Joseph Iavarone

Digitally signed under
ESRA by Joseph Iavarone
on 5/29/2020 1:12 PM

Joseph Iavarone
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 44106

Reviewed by:

Frank Sgarlata

Digitally signed under
ESRA by Frank Sgarlata
on 6/1/2020 1:46 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

TECHNICIAN TEST

SOLVAY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 138506





Date: 05/29/2020

OPERATOR NAME:
 JOSEPH A IAVARONE
 Permit #: 44106
 Operator Agency/Dept: SOLVAY VILLAGE PD
 Reference Standard #: 19281

Nominal = 0.100 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.000 | 10:29 |
| INTERNAL STANDARD | VERIFIED | 10:29 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.101 | 10:29 |
| BLANK TEST | 0.000 | 10:30 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.102 | 10:30 |
| BLANK TEST | 0.000 | 10:31 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.102 | 10:32 |
| BLANK TEST | 0.000 | 10:32 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.100 | 10:33 |
| BLANK TEST | 0.000 | 10:34 |

Average = 0.1013
 Std Dev = 0.0010

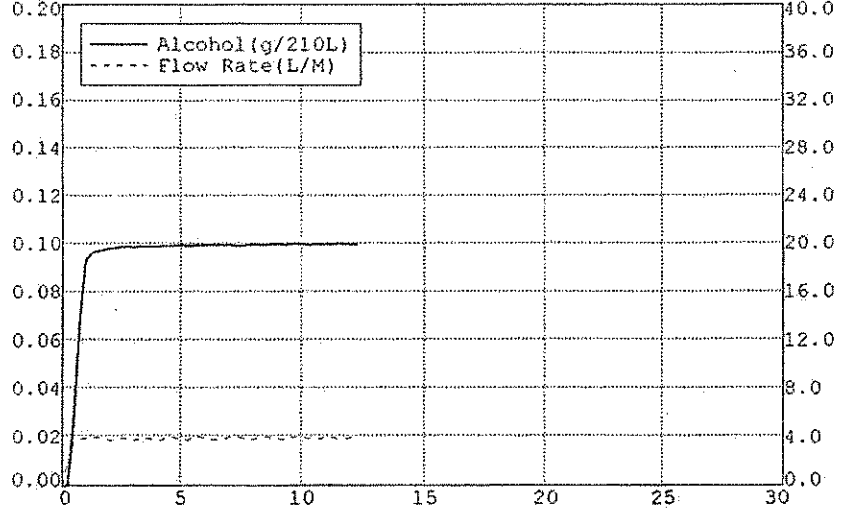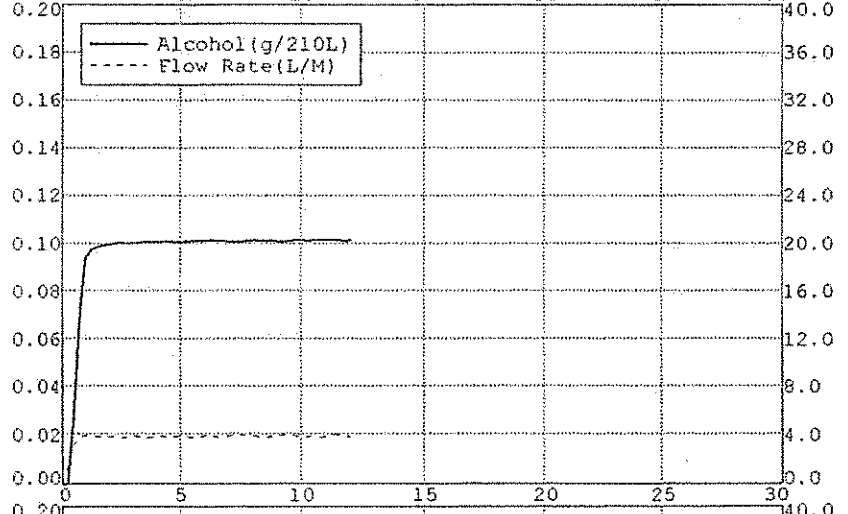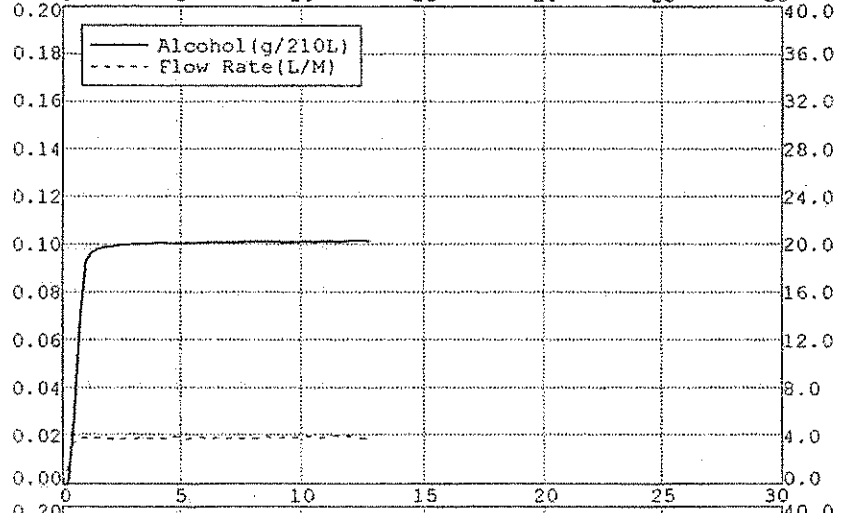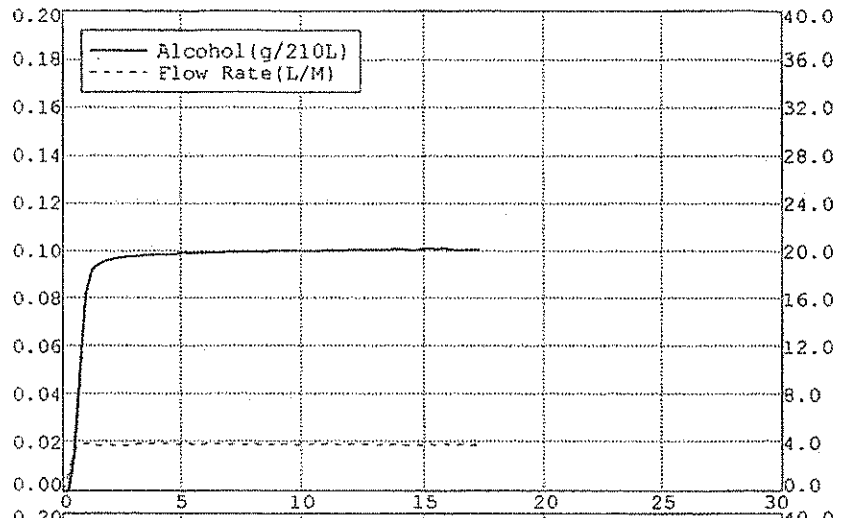

TECHNICIAN TEST

SOLVAY VILLAGE
POLICE DEPT
DATAMASTER dmt: 138506





Date: 05/29/2020

OPERATOR NAME:
JOSEPH A IAVARONE
Permit #: 44106
Operator Agency/Dept: SOLVAY VILLAGE PD
Reference Standard #: 20020

Nominal = 0.080 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.000 | 11:23 |
| INTERNAL STANDARD | VERIFIED | 11:23 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.082 | 11:23 |
| BLANK TEST | 0.000 | 11:24 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.082 | 11:24 |
| BLANK TEST | 0.000 | 11:25 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.082 | 11:26 |
| BLANK TEST | 0.000 | 11:26 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.082 | 11:27 |
| BLANK TEST | 0.000 | 11:28 |

Average = 0.0820
Std Dev = 0.0000

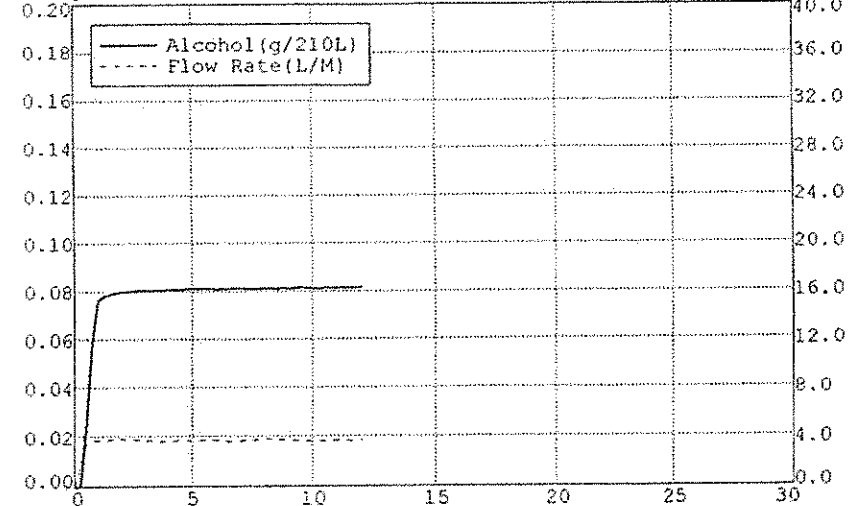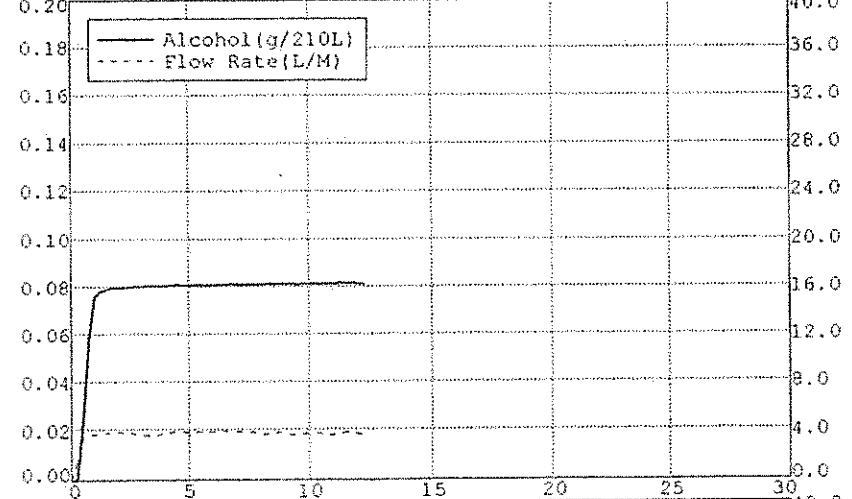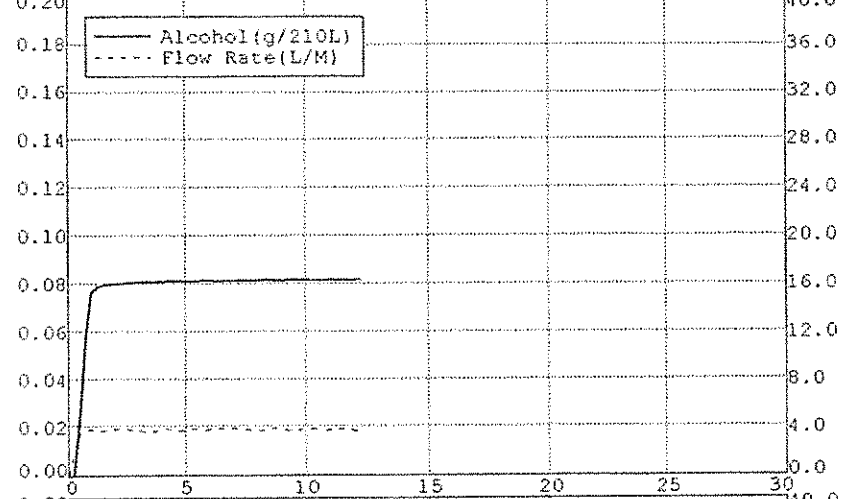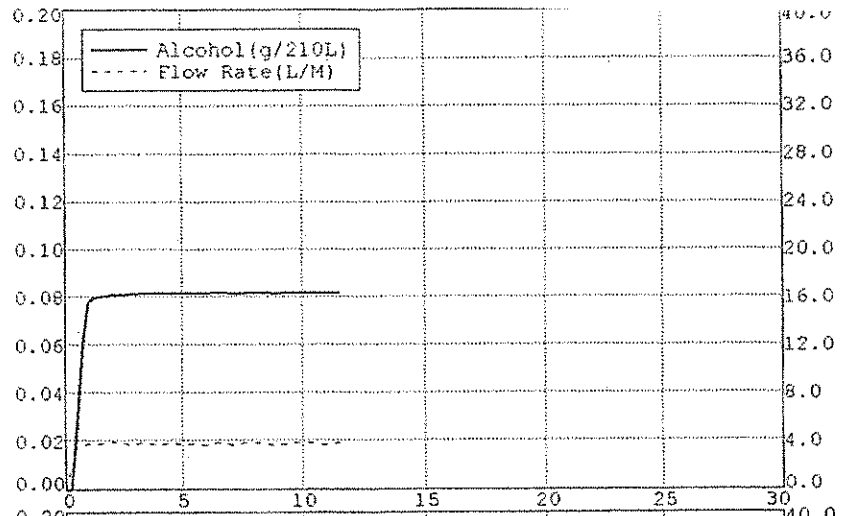

TECHNICIAN TEST

SOLVAY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 138506





Date: 05/29/2020

OPERATOR NAME:
 JOSEPH A IAVARONE
 Permit #: 44106
 Operator Agency/Dept: SOLVAY VILLAGE PD
 Reference Standard #: 19210

Nominal = 0.180 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.000 | 11:31 |
| INTERNAL STANDARD | VERIFIED | 11:31 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.185 | 11:32 |
| BLANK TEST | 0.000 | 11:32 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.185 | 11:33 |
| BLANK TEST | 0.000 | 11:34 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.186 | 11:34 |
| BLANK TEST | 0.000 | 11:35 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.186 | 11:35 |
| BLANK TEST | 0.000 | 11:36 |

Average = 0.1855
 Std Dev = 0.0006

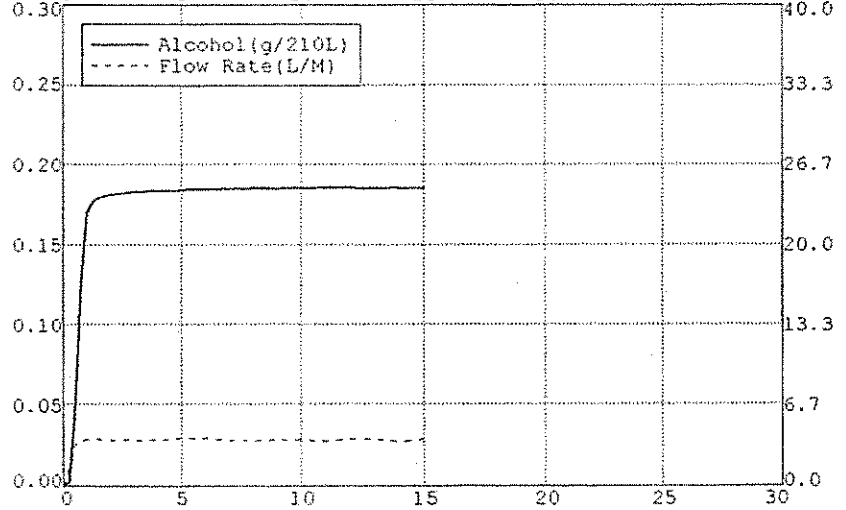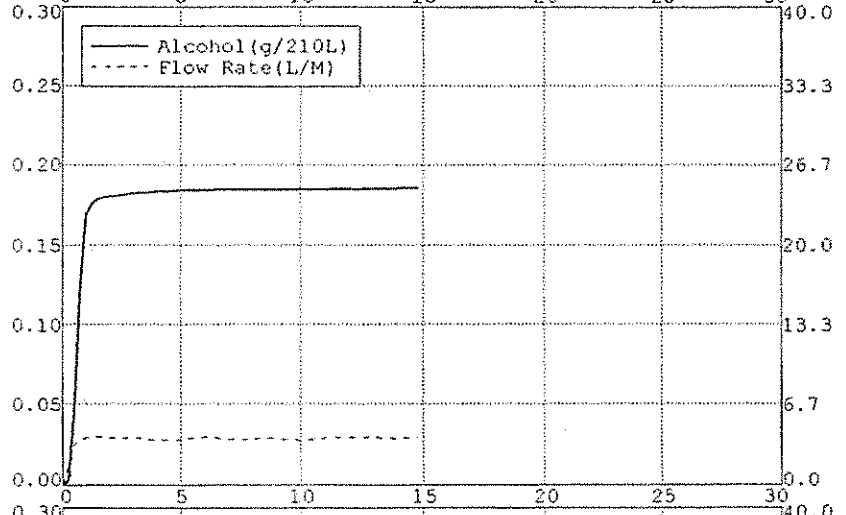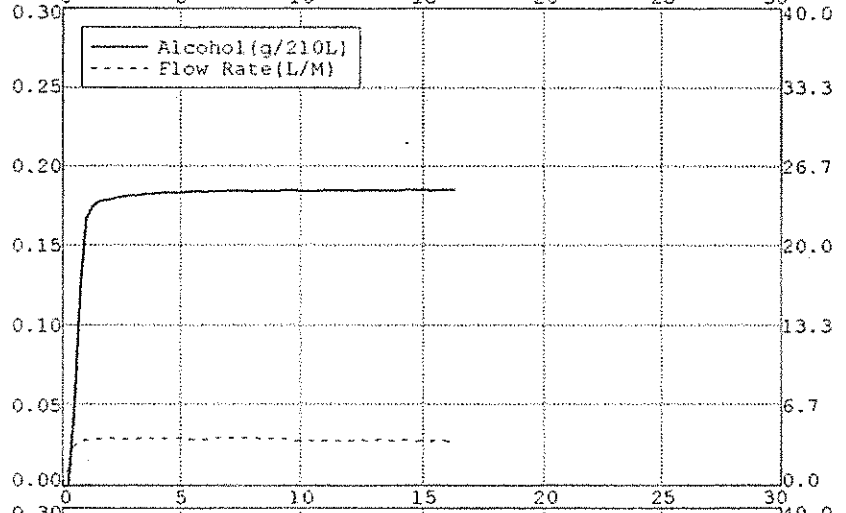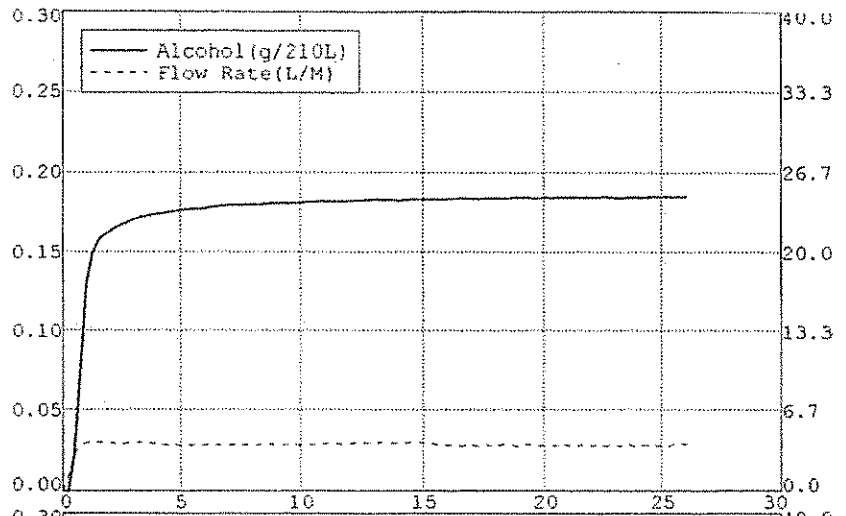


SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
80 South Swan Street
Albany, NY 12210
Ph: 518-485-7636 / 518-402-0689
Fax: 518-457-6869

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

| | | |
|---|---|---------------------------------|
| Name of Agency Solvay Police Dept | | Today's Date 05/29/20 |
| Address 507 Charles Ave | City, State, ZIP Solvay NY 13209 | |
| Contact Person ofc Nerber | Contact Telephone 315-468-2510 | |
| Contact Email | Best Way to Reach You During Appointment Period | |

SECTION II - INSTRUMENT INFORMATION

| | | | | | |
|--|--|--|---|--|--|
| Instrument Manufacturer (Please Circle) NPAS DMT REPCO SIM Applied Concepts(Stalker) Decatur(Genesis) Kustom(Eagle/Falcon) MPH A/S FST Other: | | | | | |
| Model Number DMT | | | Instrument Serial Number 138506 | | |
| Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 -- | | | | Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair | |
| Brief Description of Malfunction | | | | | |
| List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle) | | | | | |
| DMT/SIM: DMT SIM Tubes Keyboard Other: | | | Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other: | | |
| <i>I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.</i> | | | | | |
| Signature  | | | | Date 5-29-20 | |

DCJS USE ONLY

inspected instrument, checked setup voltages, print and remote operation. performed calibration and adjustment procedure on subject, technician on diagnostic tests verified calibration.