

2023

DATAMASTER

RECORD OF INSPECTION

MAINTENANCE

CALIBRATION

MAY 2023

05/04/2023



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, **Steven J. Carluccio**, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 138506, performed on May 04, 2023 by Office of Public Safety employee Joseph Iavarone, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA
by Steven J. Carluccio
on 05/12/2023 09:31 AM

Steven J. Carluccio
Highway Safety Equipment Technical Supervisor
Office of Public Safety

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Solvay Village Police Department
Manufacturer: NATL PATENT ANALYTICAL SYSTEM
Model: DATAMASTER DMT
Serial Number: 138506
Date: May 04, 2023


Reference Solution Lot Number : 23030
Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.101 %	33.99 degrees centigrade
2	0.102 %	33.99 degrees centigrade
3	0.102 %	33.99 degrees centigrade
4	0.102 %	33.99 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 138506, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA
by Joseph Iavarone
on 05/04/2023 11:33 AM

Reviewed by:



Digitally signed under ESRA
by Frank Sgarlata
on 05/04/2023 12:16 PM

Joseph Iavarone
Highway Safety Equipment Technician
Breath Analysis Operator Permit #44106

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Solvay Village Police Department
Manufacturer: NATL PATENT ANALYTICAL SYSTEM
Model: DATAMASTER DMT
Serial Number: 138506
Date: May 04, 2023

- 1. General appearance and condition of this device -----: N/A

- 2. Check controls and indicators -----: OK

- 3. Check breath flow system -----: OK

- 4. Check printer operation -----: N/A

- 5. System cycles through all modes -----: OK

- 6. Record any repairs made to this instrument and list services provided : **CHECKED REMOTE OPERATION, RAN DIAGNOSTIC AND TECHNICIAN TESTS, VERIFIED CALIBRATION.**



Performed by:

Digitally signed under ESRA
by Joseph Iavarone
on 05/04/2023 11:33 AM

Reviewed by:

Digitally signed under ESRA
by Frank Sgarlata
on 05/04/2023 12:16 PM

Joseph Iavarone
Highway Safety Equipment Technician
Breath Analysis Operator Permit #44106

Frank Sgarlata
Breath Analysis Technical Supervisor

SOLVAY VILLAGE
POLICE DEPT
DATAMASTER dmt: 138506

Date: 05/04/2023

Nominal = 0.100 g/210L

BLANK TEST	0.000	10:38
INTERNAL STANDARD	VERIFIED	10:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.101	10:39
BLANK TEST	0.000	10:39
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.102	10:40
BLANK TEST	0.000	10:41
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.102	10:41
BLANK TEST	0.000	10:42
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.102	10:42
BLANK TEST	0.000	10:43

Average = 0.1017
Std Dev = 0.0005

Control Test Record

Serial Number: 138506
Test Date: 05/03/2023 15:51:49
Location: 190

SOLVAY VILLAGE POLICE DEPT.

Supervisor Information

First Name: Tyler R
Last Name: Hemingway
Permit: 49966
Agency: SOLVAY VILLAGE PD

Simulator Information


Lot: 23030 Nominal: 0.100

Test Results

Alcohol 1: 0.10 33.99
Alcohol 2: 0.10 33.99
Alcohol 3: 0.10 33.99

Solution Change:

Plot 1 of 3

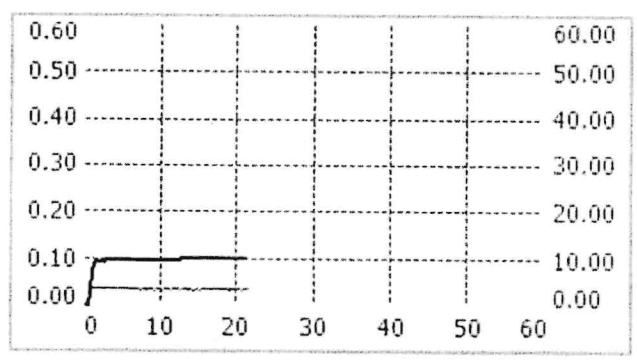

Status

Status Code:
Date Time:
Message:

2023

DATAMASTER (138506)

SIMULATOR (MP4078)

RECORD OF INSPECTION

MAINTENANCE

CALIBRATION

NOVEMBER 2023

11/27/2023



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, **Steven J. Carluccio**, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 138506, performed on November 27, 2023 by Office of Public Safety employee Martin Schilling, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA
by Steven J. Carluccio
on 12/05/2023 08:33 AM

Steven J. Carluccio
Highway Safety Equipment Technical Supervisor
Office of Public Safety

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Solvay Village Police Department

Manufacturer: NATL PATENT ANALYTICAL SYSTEM

Model: DATAMASTER DMT

Serial Number: 138506

Date: November 27, 2023

Reference Solution Lot Number : 23050

Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.100 %	34.01 degrees centigrade
2	0.100 %	34.00 degrees centigrade
3	0.101 %	34.00 degrees centigrade
4	0.101 %	34.01 degrees centigrade

Reference Solution Lot Number : 23100

Reference Solution Standard : 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.080 %	34.01 degrees centigrade
2	0.080 %	34.00 degrees centigrade
3	0.080 %	34.01 degrees centigrade
4	0.080 %	34.01 degrees centigrade

Reference Solution Lot Number : 23380


Reference Solution Standard : 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.178 %	34.00 degrees centigrade
2	0.179 %	34.01 degrees centigrade
3	0.179 %	34.00 degrees centigrade
4	0.180 %	34.00 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 138506, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:

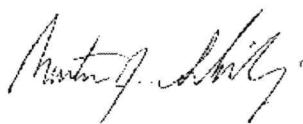

Digitally signed under ESRA
by Martin Schilling
on 11/27/2023 12:46 PM

Reviewed by:

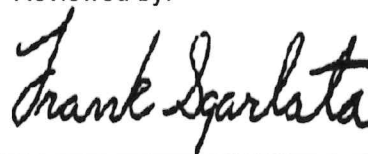

Digitally signed under ESRA
by Frank Sgarlata
on 11/27/2023 01:46 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45926

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Solvay Village Police Department
Manufacturer: NATL PATENT ANALYTICAL SYSTEM
Model: DATAMASTER DMT
Serial Number: 138506
Date: November 27, 2023

- 1. General appearance and condition of this device -----: OK

- 2. Check controls and indicators -----: OK

- 3. Check breath flow system -----: OK

- 4. Check printer operation -----: OK

- 5. System cycles through all modes -----: OK

6. Record any repairs made to this instrument and list services provided : **INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**



Performed by:

Digitally signed under ESRA
by Martin Schilling
on 11/27/2023 12:46 PM

Reviewed by:

Digitally signed under ESRA
by Frank Sgarlata
on 11/27/2023 01:46 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit #45926

Frank Sgarlata
Breath Analysis Technical Supervisor

TECHNICIAN TEST

SOLVAY VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 138506


Date: 11/27/2023

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: SOLVAY VILLAGE PD
 Reference Standard #: 23100

Nominal = 0.080 g/210L

BLANK TEST	0.000	09:48
INTERNAL STANDARD	VERIFIED	09:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	09:49
BLANK TEST	0.000	09:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	09:50
BLANK TEST	0.000	09:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	09:51
BLANK TEST	0.000	09:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	09:52
BLANK TEST	0.000	09:53

Average = 0.0800
 Std Dev = 0.0000

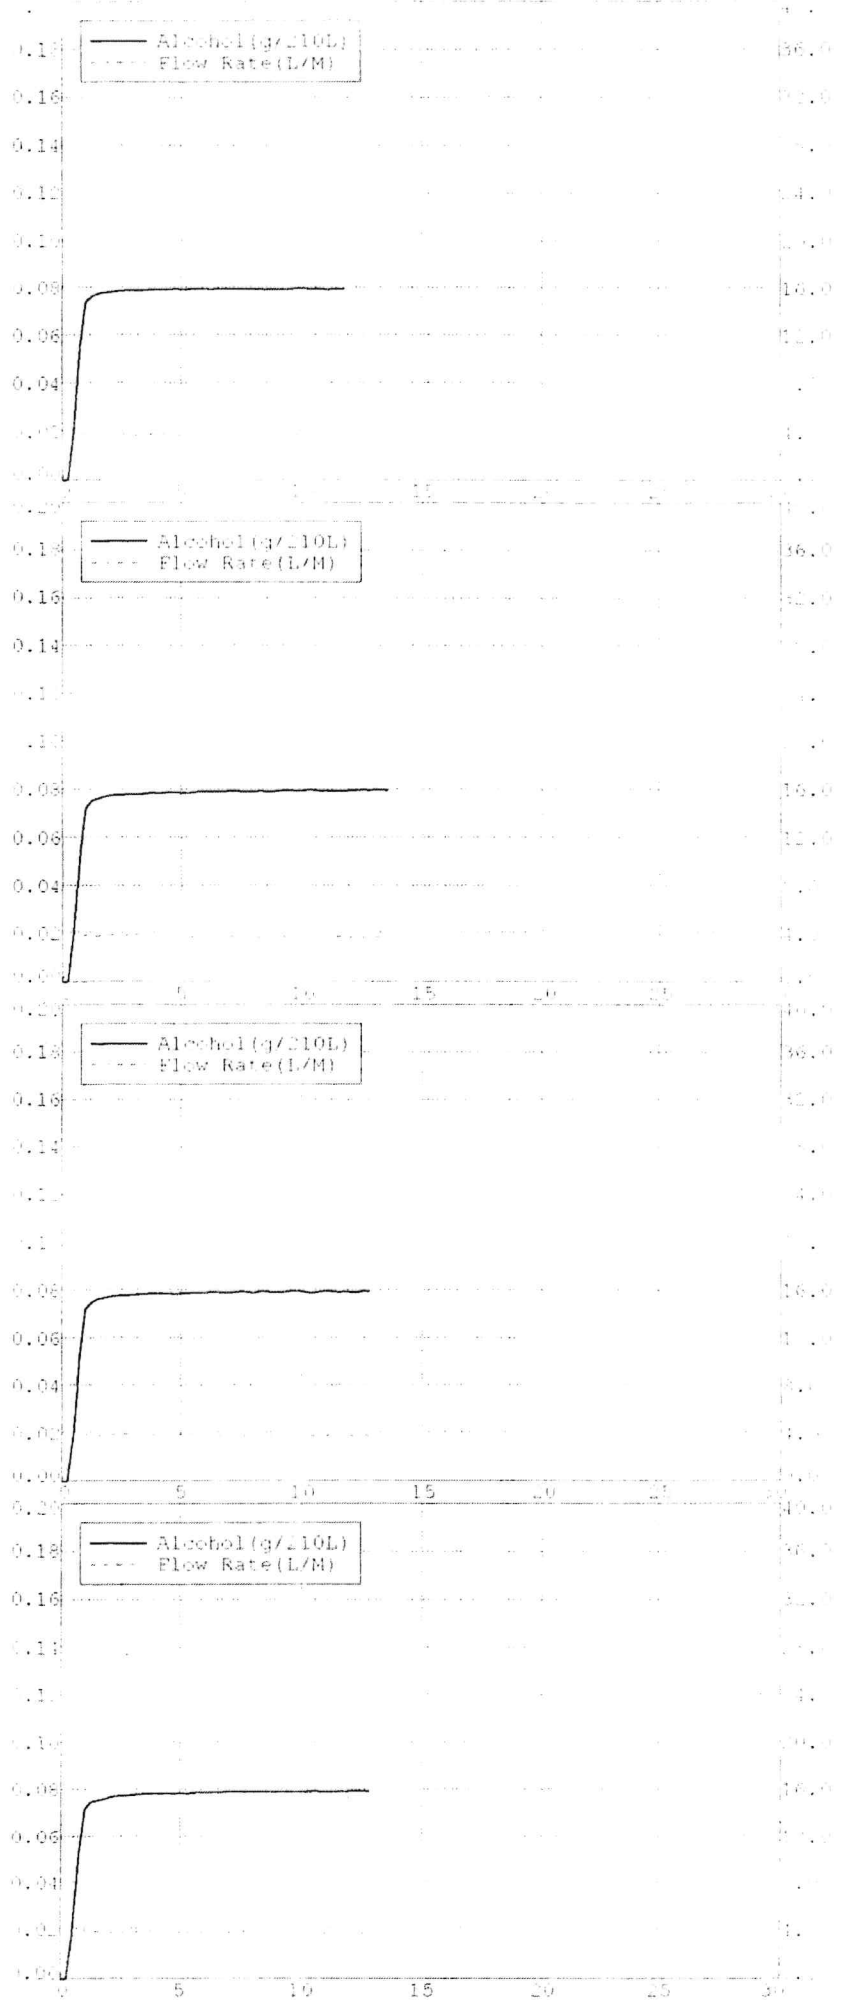

TECHNICIAN TEST

SOLVAY VILLAGE
POLICE DEPT
DATAMASTER dmt: 138506





Date: 11/27/2023

OPERATOR NAME:
MARTIN J SCHILLING
Permit #: 45926
Operator Agency/Dept: SOLVAY VILLAGE PD
Reference Standard #: 23050

Nominal = 0.100 g/210L

BLANK TEST	0.000	09:23
INTERNAL STANDARD	VERIFIED	09:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.100	09:23
BLANK TEST	0.000	09:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.100	09:24
BLANK TEST	0.000	09:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	09:26
BLANK TEST	0.000	09:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.101	09:27
BLANK TEST	0.000	09:28

Average = 0.1005
Std Dev = 0.0006

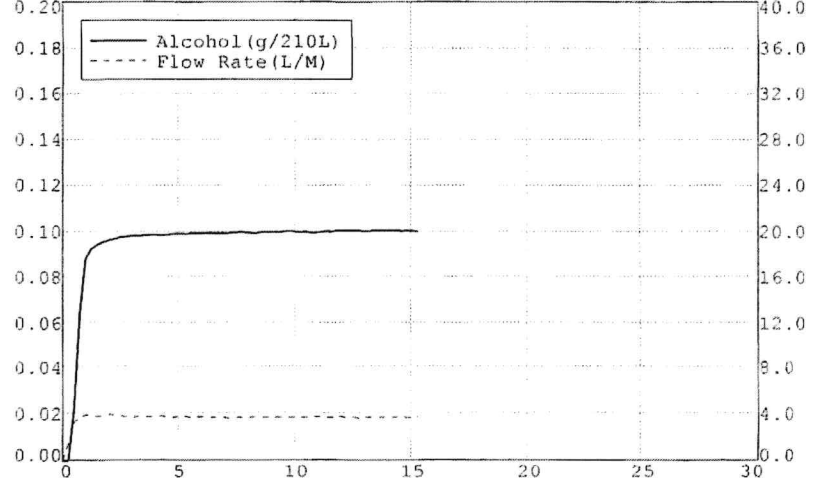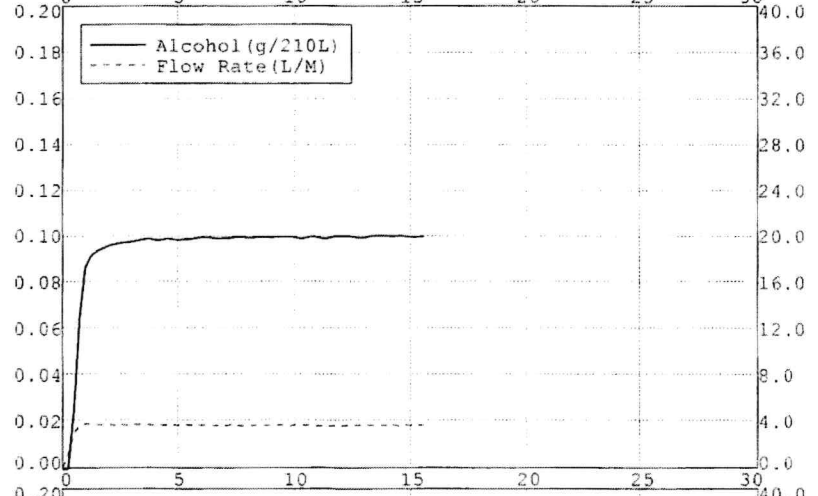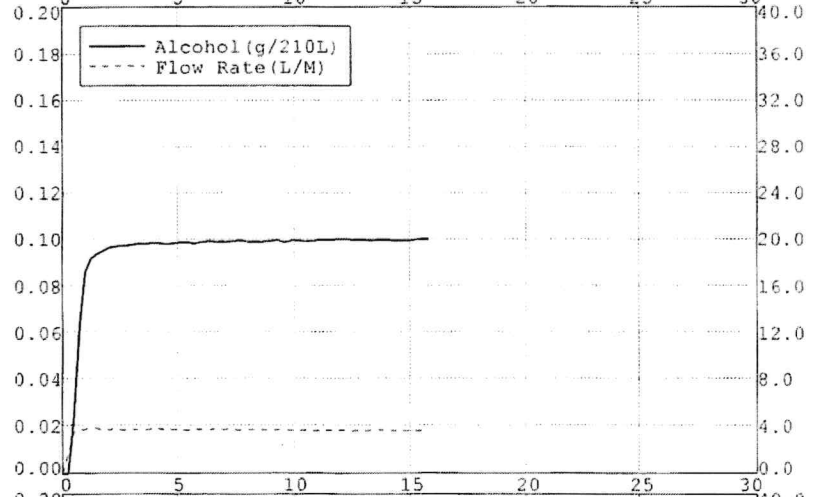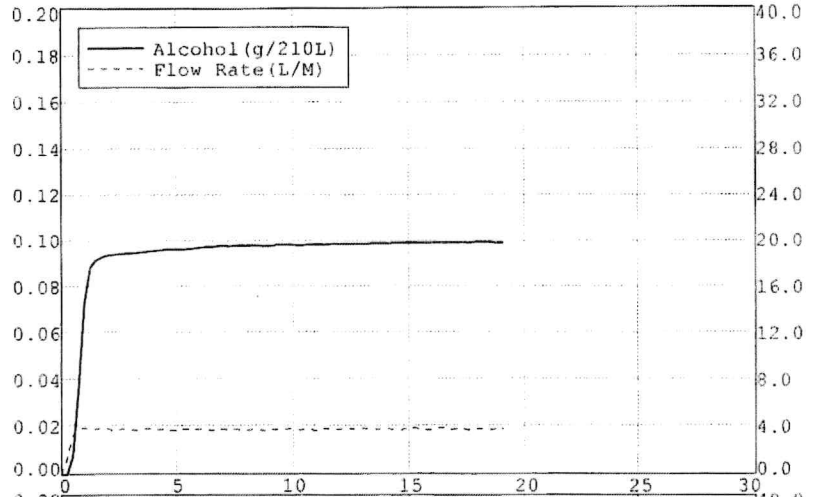

TECHNICIAN TEST

SOLVAY VILLAGE
POLICE DEPT
DATAMASTER dmt: 138506


Date: 11/27/2023

OPERATOR NAME:
MARTIN J SCHILLING
Permit #: 45926
Operator Agency/Dept: SOLVAY VILLAGE PD
Reference Standard #: 23380

Nominal = 0.180 g/210L

BLANK TEST	0.000	10:06
INTERNAL STANDARD	VERIFIED	10:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.178	10:06
BLANK TEST	0.000	10:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.179	10:08
BLANK TEST	0.000	10:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.179	10:09
BLANK TEST	0.000	10:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.180	10:10
BLANK TEST	0.000	10:11

Average = 0.1790
Std Dev = 0.0008

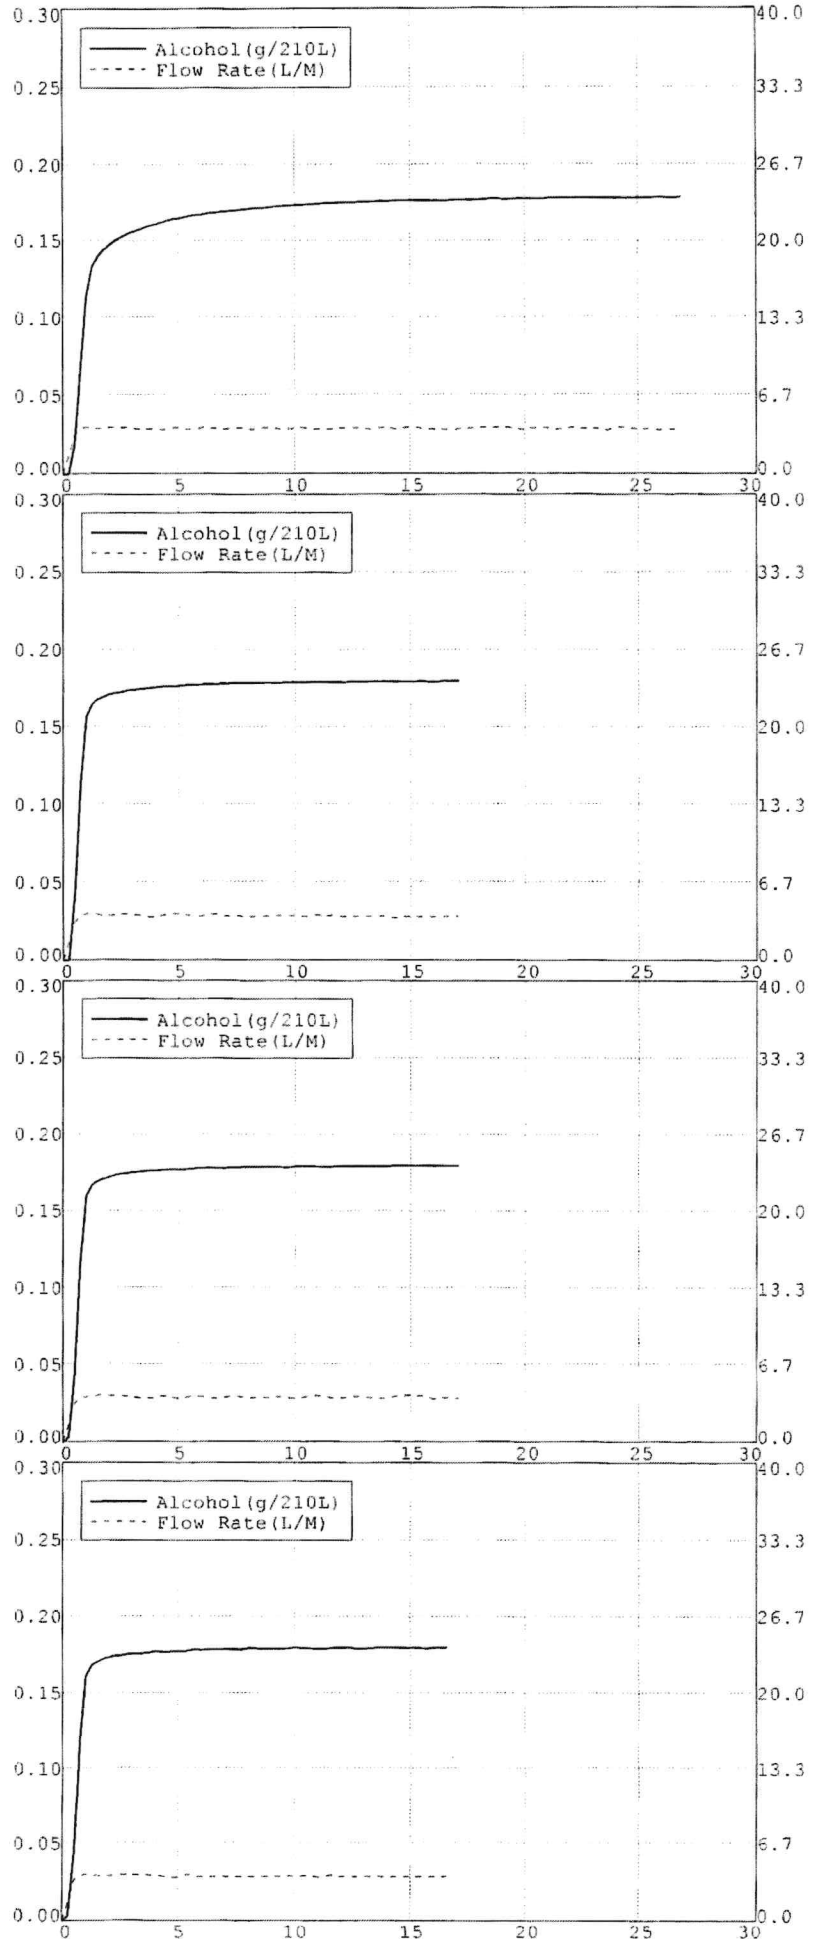

SERVICE AUTHORIZATION FORM
 Highway Safety Technology Unit
 80 South Swan Street
 Albany, NY 12210
 Ph: 518-485-7636 / 518-402-0689
 Fax: 518-457-6869

MJ
11/27/23

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

Name of Agency Solvay Police Dept.	Today's Date 11/27/2023
Address 507 Charles Ave	City, State, ZIP Solvay NY 13209
Contact Person Ofc. Hemingway	Contact Telephone 315-468-2510
Contact Email themingway@solvaypd.com	Best Way to Reach You During Appointment Period

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) <input checked="" type="radio"/> NPAS DMT <input type="radio"/> GUTH <input type="radio"/> Applied Concepts (Stalker) <input type="radio"/> Decatur (Genesis) <input type="radio"/> Kustom (Eagle/Falcon) <input type="radio"/> MPH <input type="radio"/> Alco-Sensor <input type="radio"/> Other:		
Model Number <i>Datanuster DMT</i>	Instrument Serial Number <i>138506</i>	
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --	Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: <input checked="" type="radio"/> DMT <input type="radio"/> SIM <input checked="" type="radio"/> Tubes <i>1 Brent's hose</i> <i>1 Jam Tubes</i> <input type="radio"/> Keyboard Other: <i>Power cords</i>	Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other: _____	
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.		
Signature <i>Ofc. T. W...</i> #0024	Date <i>11/27/23</i>	

DCJS USE ONLY

I inspected instrument. Checked settings, multimeter printouts and search operation. I performed calibration / adjustment procedure. Per subject, tubing and diagnostic tests. Verified calibration.



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Steven J. Carluccio, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of GUTH LABORATORIES, 12V500 SIMULATOR, serial number MP4078, performed on November 27, 2023 by Office of Public Safety employee Martin Schilling, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA
by Steven J. Carluccio
on 12/05/2023 07:40 AM

**Steven J. Carluccio
Highway Safety Equipment Technical Supervisor
Office of Public Safety**

**SIMULATOR
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Solvay Village Police Department

Manufacturer: GUTH LABORATORIES

Model: 12V500

Serial Number: MP4078

Date: November 27, 2023

Breath Simulator Temperature
34.01 degrees centigrade



Division of Criminal
Justice Services

I hereby certify that I have performed any necessary maintenance procedures and verified the calibration of GUTH LABORATORIES simulator model 12V500, serial number MP4078, and have determined that it is accurate.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified simulator was performed, or within a reasonable time thereafter.

A handwritten signature in black ink that reads "Martin Schilling".

Digitally signed under ESRA
by Martin Schilling
on 11/27/2023 12:44 PM

**Martin Schilling
Highway Safety Equipment Technician
Office of Public Safety**

**SIMULATOR
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Solvay Village Police Department
Manufacturer: GUTH LABORATORIES
Model: 12V500
Serial Number: MP4078
Date: November 27, 2023

- 1. General appearance and condition of this device -----: OK**

- 2. Check propeller rotation -----: OK**

- 3. Check for air leaks -----: OK**

- 4. Check for proper temperature -----: OK**

5. Record any repairs made to this instrument and list services provided : VERIFIED CALIBRATION



Division of Criminal
Justice Services

A handwritten signature in black ink that reads "Martin G. Schilling".

Digitally signed under ESRA
by Martin Schilling
on 11/27/2023 12:44 PM

Martin Schilling
Highway Safety Equipment Technician
Office of Public Safety

NIST Traceable
Calibration Report

REPORT NUMBER

1722185

625 East Bunker Court
 Vernon Hills, Illinois 60061
 PH: 866-466-6225
 Fax: 847-327-2993
 www.innocalsolutions.com

Reference Number: 136536200
 PO Number: SCARLUCCIO030823

NY State Div Of Criminal Justice Svcs
 80 South Swan Street
 Albany, NY 12210 United States

Manufacturer:	Alpha Technics	Calibration Date	03/28/2023
Model Number:	91-5443	Calibration Due Date	03/28/2024
Description:	Temperature, Thermometer	Condition As Found:	In Tolerance
Asset Number:	20BMM01712	Condition As Left:	In Tolerance, No adjustment
Serial Number:	20BMM01712		
Procedure:	DS Alpha Technics 5000 Series f/NY State DCJS		

Remarks:
 NIST-traceable calibration performed on the unit referenced above in accordance with customer requirements, published specifications and the lab's standard operating procedures. No adjustments were made to the unit.

Standards Used

Standard ID	Manufacturer	Model Number	Description	Cal Date	Due Date
CP106957	Hart Scientific	5699	Temperature, Probe, SPRT	3/19/2021	4/30/2023
CP32033	Hart Scientific	5628	Temperature, Probe	5/24/2021	3/31/2023
CP32034	Hart Scientific	5628	Temperature, Probe	11/16/2021	5/31/2023
CP50205	Hart Scientific	5628	Temperature, Probe	3/16/2022	9/30/2023
CP50219	Hart Scientific	1590	Temperature, Super Thermometer	3/10/2021	3/31/2023

Calibration Data

Function Tested	Nominal / Reference Value	Measured Value	OOT	Calibration Tolerance <i>g: = Guard Banding Applied</i>	TUR	EMU
Temperature	-15.000 °C					
As Found & As Left	-15.000	-14.99		-15.050 to -14.950 °C	4.3:1	± 0.012 °C
	0.000 °C					
As Found & As Left	0.000	0.00		-0.030 to 0.030 °C	4.1:1	± 0.0074 °C
	75.000 °C					
As Found & As Left	75.000	75.00		74.970 to 75.030 °C	2.7:1	± 0.011 °C
	125.000 °C					
As Found & As Left	125.000	124.96		124.950 to 125.050 °C	3.9:1	± 0.013 °C

Temperature: 23 °C
 Humidity: 37 %RH
 Rpt. No.: 1722185

Calibration Performed By:		Quality Reviewer:	
Mary Paschen	Metrologist	Jeff Ziegler	3/28/2023
Name	Title	Name	Date

This report may not be reproduced, copied in full, without written permission of Innocal. The results stated in this report relate only to the item(s) tested or calibrated. Measurements reported herein are traceable to SI units via national standards maintained at NIST and were performed in compliance with MIL-STD-45662A, ANSI/NCSL Z540-1:1994, 10GPR50, Appendix B, ISO 9002:94, and ISO 17025:2017. Confirmation of Calibration Acceptance as a Decision Rule. The estimated measurement uncertainty (EMU), if reported in this certificate, is being reported at a confidence level of 95% (K=2) unless otherwise noted in the remarks section.

SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
 80 South Swan Street
 Albany, NY 12210
 Ph: 518-485-7636 / 518-402-0689
 Fax: 518-457-6869

*MJ
11/27/23*

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

Name of Agency Solvay Police Dept.		Today's Date 11/27/2023
Address 507 Charles Ave		City, State, ZIP Solvay NY 13209
Contact Person Ofc. Hemingway		Contact Telephone 315-468-2510
Contact Email themingway@solvaypd.com		Best Way to Reach You During Appointment Period

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) NPAS DMT GUTH Applied Concepts (Stalker) Decatur (Genesis) Kustom (Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number 12V500	Instrument Serial Number 53300 <i>MP 4078</i>	
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --	Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: DMT SIM Tubes Keyboard Other: sim holder	Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other:	
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.		
Signature <i>Ofc T. [unclear] #0024</i>		Date 11/27/23

DCJS USE ONLY

Export °C <u>33.99</u> <u>33.99</u> <u>33.99</u>	Digital °C <u>34.01</u> <u>34.01</u> <u>34.01</u>	Thermometer: <u>208MM01712</u> Calibration Due: <u>3-28-24</u> Air Leak Test: <u>OK</u> Propeller Rotation: <u>OK</u>
---	--	---